



DV-50

LED Light Curing Device

OPERATION MANUAL

Manufacturer Name: Guilin Veirun Medical Technology Co., Ltd.

Address: No. D-07 Information Industry District, High-Tech Zone,

541004 Guilin, Guangxi, PEOPLE'S REPUBLIC OF CHINA

Tel: +86(773)5880619 Fax: +86(773)2260519

Web: www.veirun.com E-mail: info@veirun.com



Shanghai International Holding Corp. GmbH (Europe)

Eiffestrasse 80, 20537 Hamburg, Germany

Tel: +49-40-2513175/+49 163 6233205

E-mail: shholding@hotmail.com

Rev.06/2023
File No.: DVP050000084
Date of compilation: 2023/6/28
Period of use: 8 years



Guilin Veirun Medical Technology Co., Ltd.

Contents

Copyright and Notice	1
1. Introduction.....	2
2. Structure.....	2
3. Technical Specifications.....	3
4. Mounting and Dismounting.....	4
5. Operating Instructions.....	5
6. Precautions.....	7
7. Contraindications and applicable groups.....	8
8. Maintenanc.....	9
9. Trouble Shooting.....	9
10. Storage and Transportation.....	10
11. After-sale Service.....	10
12. Environmental Protection.....	10
13. Symbol Instructions.....	11
14. Statement.....	11
15. Attachment Lists.....	12
16. EMC.....	12

Copyright and Notice

Guilin Veirun Medical Technology Co.,Ltd. All rights reserved.

Congratulations on your becoming a distinguished customer of Veirun, welcome to use DV-50 LED Curing Light, it will bring you a new experience and convenience.

This manual is compiled according to the relevant laws and regulations of China and the specific conditions of the DV-50 LED Curing Light manufactured by Guilin Veirun Medical Technology Co.,Ltd.

This manual contains the latest information as of the printing of this manual. Guilin Veirun Medical Technology Co.,Ltd. is solely responsible for the revision and explanation of the simplified English version of this manual, and reserves the right to change the relevant content after printing this manual without prior notice.

The pictures involved in this manual are schematic diagrams and are for reference only. If the pictures do not match the actual objects, the actual objects shall prevail.

All materials in this manual are protected by copyright law. Without the prior written consent of Guilin Veirun Medical Technology Co.,Ltd.,any content in the manual shall not be reproduced, copied or translated into other languages in any form.

The operator must operate in strict accordance with the operating instructions of this manual. Otherwise, Guilin Veirun Medical Technology Co.,Ltd. is not responsible for any errors and instrument failures caused by illegal operations.

Notice: Guilin Veirun Medical Technology Co.,Ltd. does not promise that the instrument is used for a particular purpose and makes any implied warranties for its merchantability and applicability.

If you need after-sales service support, please contact Guilin Veirun Medical Technology Co., Ltd. or an authorized agent.

1 Introduction

1.1 Principles of operation

The device illuminates photosensitive resin to solidify it quickly based on the principle of light radiation.

1.2 Intended use


The device is intended to be used on a variety of dental compositions within the oral cavity.

1.3 Features

- Stable output power guarantees constant light so that the solidification effect is not affected by the consumption of remaining power.
- Parallel light ensures more focused output energy and better solidification effect.
- Super capacity battery. A full charge can be used for more than 500 times continuously under 10s working of P2 mode,from full charge to low-battery alert.
- Ergonomics design, excellent and comfortable handle feel during the treatment.
- Aluminum alloy body, resistance to shatter and drop.
- Light source featuring 360-degree rotation to realize curing from all directions.
- Replaceable light source and enables detection of dental caries.
- Charger verifying radiation output of LED light curing device effective or not.
- Solidified lens fixed on light source,bonded with all-ceramic veneer and adhered to crown and fiber-reinforced composite root canal post to make solidification effect better.
- Replaceable Lithium battery, Auto power-off.

2 Structure

LED Light Curing Device consists of main unit, charger cradle, battery, light guide, shading plate and power adapter.

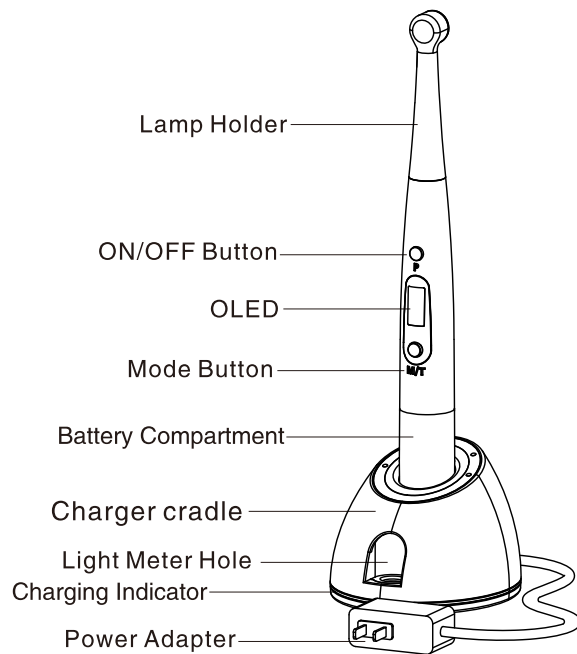

3 Technical Specifications

3.1 Dimensions: $\phi 22.5 \text{ mm} \times 217 \text{ mm}$.

3.2 Main unit net weight: 117 g.

3.3 Configurations: see the packing list for details.

3.4 Power supply:

- Power supply classification:
Power supply by rechargeable lithium battery.
- Rechargeable lithium battery:
Standard voltage: DC3.6 V, capacity: 2000 mAh,
with protection for overvoltage, overcurrent and short-circuits.

Power Adapter:

Power Adapter :

Input : 100V–240V~, 50/60 Hz, 22VA

Output : 5V=1A.

Fuse: T1AL 250 V.

3.5 Characteristics of LED lamp:

10 W high-power blue LED lamp

Lamp classification group: Risk Group 2.

Wavelength: 385 nm~515 nm.

Inspection method: When the LED lamp emits during normal operation, the lamp is in good condition.

Radiation during continuous working: $\geq 400 \text{ mW/cm}^2$.

Optical effective area of light source: 75 mm^2 .

It is applicable to some common dental resinous materials in clinic, such as 3 M, Dentsply etc.

3.6 Working environment:

Temperature: $5^\circ\text{C} \sim 40^\circ\text{C}$, Relative humidity: $\leq 80\%$,

Atmospheric pressure: 75 kPa~106 kPa.

Equipment Safety classification:

Operation mode: Short-time operation equipment.

Type of protection against electric shock: Class II equipment.

Degree of protection against electric shock: Type B applied part.


Degree of protection against ingress of water: Ordinary equipment (IPX0).

Degree of safety of application in the presence of a Flammable Anesthetic Mixture with air, Oxygen or Nitrous Oxide: Non-AP, APG type equipment.

4 Mounting and Dismounting


4.1 The top of the body unit featuring 360° rotation is replaceable.

As shown in figure.



4.2 Battery Replacement

Holding the front of the host and the battery compartment, screw it off counterclockwise, then remove the old battery from the battery, change a new battery, and then replace the battery storehouse on the host. The battery positive and negative can be normal used, no security risks. As shown in figure:

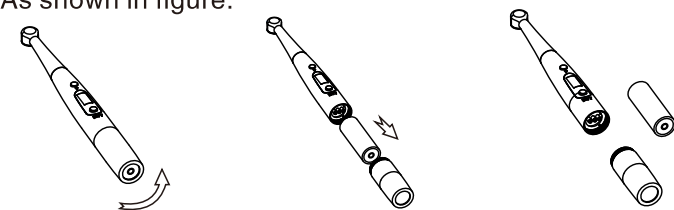

4.3 Press and install the shading sheet on the light guide head.

4.4 When the battery needs to be charged, connect the USB Type A jack into the plug of the adapter and connect the plug of the adapter into the AC100V–240V power supply. Then connect the Micro USB of the USB cable to plug of the pedestal. Put the main unit to the charging point of the pedestal, and the curing light starts charging.

5 Operating Instructions

5.1 Press button "M/T" for 1 second and release the button when the buzzer warns for once. Following three modes are available.

(Not selectable in caries detection mode, only used for detection).

- Full Power Mode: The screen shows "П", The output light intensity is full-power. (recommended mode for clinical).
- Progressive Mode: The screen shows "Л", The output light intensity enhances gradually, power output is to maximum after 5 seconds.
- Pulsed Mode: The screen shows "п п", The blue light works in pulse manner.


5.2 Press button "M/T" for 2 second and release the button when the buzzer warns for twice. Following four modes based on output of power density are available.

- Ultra High Power Density: The screen shows "P1", The power density is about $2300 \text{ mW/cm}^2 \sim 2600 \text{ mW/cm}^2$.
- High Power Density: The screen shows "P2", The power density is about $1600 \text{ mW/cm}^2 \sim 1900 \text{ mW/cm}^2$.
- Standard Power Density: The screen shows "P3", The power density is about $1000 \text{ mW/cm}^2 \sim 1300 \text{ mW/cm}^2$.
- Caries Detection Power Density: The screen shows "P4" and "CHECK", and the purple light is output independently. The purple light works under proper use can be regarded as normal.

5.3 Tap button "M/T" to select working time interval.

- In "P3" mode, the time interval can be chose from 1, 2, 3, 4, 5, 10, 15, 20, 25, 30, 35, 40 second.
- In "P2" mode, the time interval can be chose from 1, 2, 3, 4, 5, 10, 15, 20 second.
- In "P1" mode, the time interval can be chose from 1, 2, 3, second.
- In "P4" mode, the time interval can not be chose.

Information on the screen is shown in the figure.

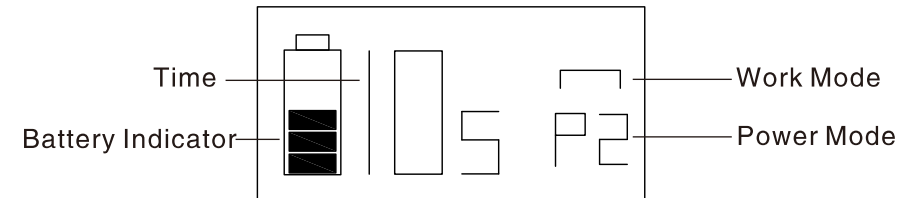

5.4 During the operation, put the disposable sleeve on the top of the main unit, aim the top at the correct position, press the ON/OFF button ("P") and the main unit will produce "Di" sound, the curing light radiates blue light and starts working according to the set modes. Meanwhile, it starts counting down from the set working time interval, it stops working when counting down to "0". The screen displays the set working time interval again.

5.5 Operation can be stopped by press the ON/OFF button ("P").

5.6 After a working cycle, operator can press the ON/OFF button ("P") to start another working cycle. Stop operating if the equipment is burning obviously, let equipment cool down before restarting. Suggest continuous working cycle less than 5 times.

5.7 Battery Indicator: Low power detective circuit is fixed inside of the main unit. If battery indicator in the screen has only 1 bar left, please charge in time.

5.8 When the battery needs to be charged, plug USB Type A jack in USB Type A plug of power adapter, and connect the plug of power adapter into the AC100V–240V power supply, and connect Micro USB of USB cable into charge indicator in charge. The blue indicator light on charger indicates

charger on standby. Put the main unit to the charging point of the charger, and the indicator light turns green, the curing light starts charging. When charging finished, the indicator light at the bottom of charger turn blue.

5.9 After operating, take off the disposable sleeve and throw away, avoid reusing. Power output will be decreased by 5–10% if using the disposable sleeve.

5.10 The product will turn off automatically if there is no operations within 2 minutes. Turn it on by pressing any button.

5.11 The depth of solidification of dental resin composite is no less than 4mm per 10 second. The recommended separation distance between luminous point and solidifying point is 2mm.

5.12 The Optometry Function

Connect the charging base to the power adapter.

- Adjust the power output mode to P3, align the light source head with the Light meter hole of the charger and keep it vertical, press the "P" On/Off key, and the charger should be able to light 1 indicator light.
- Adjust the power output mode to P2, align the light source head with the Light meter hole of the charger and keep it vertical, press the "P" On/Off key, and the charger should be able to light 2 to 4 indicator light.
- Adjust the power output mode to P1, align the light source head with the Light meter hole of the charger and keep it vertical, press the "P" ON/OFF key, and the charger should be able to light 5 indicator light.

6 Precautions

Warning: It's our duty to provide users correct usage rules and safety notices.

6.1 Using the product according to the instruction manual, other tasks are out of support.

6.2 Please charge the battery at least 4 hours before first time usage.

6.3 In order to prevent cross-infection, it is forbidden to reuse the disposable sleeve.

6.4 The top of the main unit can be turned by 360 degree and it is demountable and replaceable.

6.5 DV-50 LED light curing device only used by professionally trained people.

6.6 Please put it away from the touch of kids.

6.7 During operation, the light should be aimed straightly at the dental resin composite to ensure the effect of solidification.

6.8 Avoid aiming the light at eyes, please use brake sack or protective goggles supplied by our company to protect your eyes.

6.9 Please use the power adapter which is designed and supplied by our company. It may cause potential dangers to lithium and control circuit by using the power adapter designed or supplied by other manufacturers.

6.10 It is forbidden to put metal on the charger because it may burn the internal circuit. Unplug the plug of charger when not charging.

6.11 Please charge the battery in cool and ventilated room.

6.12 The product should not be used more than rated working time set in the instruction manual to avoid damaging teeth for the high temperature. Shut down and cool the product when it is used for 5 times continuously.

6.13 It is forbidden to extrude, shake or rock the battery. It is forbidden to self-taking apart the battery, in order not to result in short-circuit or leakage and it is forbidden to put the battery with metal.

6.14 Long time do not use the product, please take the lithium battery apart from the main unit. It is recommended that the product should be installed at the medical site where there are no high frequency high voltage equipments within 5 meters to ensure the product work properly.

7 Contraindications and applicable groups

7.1 People suffered ophthalmic surgeries or sensitive to light, pregnant women, children and the heart disease patients should not use the product.

7.2 Patients with retinal diseases should be cautious to use the product.

7.3 Patients with photosensitization and solar dermatitis or using photosensitive drugs should not use the product.

Applicable to all groups except contraindications.

8 Maintenance

8.1 This product does not consist of the self-maintainable spare parts.

The maintenance of this product should be taken by the appointed professional or special repair shop.

8.2 Users can change brake sack, light source and lithium battery. Please use accessory which is designed and supplied by our company. contact with the local dealer or our company if you want to buy. It may cause potential dangers to curing light or other damages which is designed and supplied by other manufacturers.

8.3 The accessory of the product should be cleaned by clean water or neutral sterilized liquid. Do not soak. Do not use highly volatile and diffluent solvent to clean this product, which can cause the signs on the control pane to fade.

8.4 Please check whether there are any remains on luminous point and clean the top of the main unit with 75% alcohol tampon after using to avoid pollute and ensure solidified effect.

8.5 Please charge in time when battery level is low; get lithium battery out for safe-keeping when not using the product for a long time.

9 Trouble Shooting

Faulty	Possible cause	Solutions
No indication, no responsefour	1.Battery is out of power. 2.Faulty of battery. 3.The main unit battery protection system works	1.Charge the product/change battery 2.Change battery 3.Place the main unit on the charge for activation
"Er"shown on the screen.	Faulty of main unit.	Send to after-sale service for repair.

Light intensity is weak.	There is resin on the top of the main unit.	Clear the resin.
The equipment is not charging when the adapter is connected.	1.The adapter is not connected well. 2.Faulty from adapter or incompatible. 3. The charger is out of order.	1.Reconnect. 2.Change th adapter 3.Send to after-sale service for repair.
Usage time shortened on a single full charge.	Smaller battery capacity.	Change battery.

Note: If such solutions are completed, the product still cannot work normally, please contact with the distributor or our company.

10 Storage and Transportation

10.1 The product should be handled carefully and lightly. Be sure that it is far from the vibration, and installed or kept in a cool, dry and ventilated place.

10.2 Do not store the product together with the combustible, poisonous , caustic or explosive goods. The product shall be stored at the location as follow:

- ① Relative humidity: $\leq 90\%$, ② Atmospheric pressure: 75 kPa~106 kPa,
- ③ Temperature: $-20^{\circ}\text{C}\sim 55^{\circ}\text{C}$.

10.3 During transportation, excessive shock and vibration shall be prevented, and handled carefully and lightly. Keep it away from sunlight, snow or rain. It shall not be packed with dangerous goods.


































11 After-sale Service

From the date this product has been sold, base on the warranty card, we will repair this equipment free of charge if it has quality problems, please refer to the warranty card for the warranty period.

12 Environmental Protection

There is not any harmful element in our product. It can be disposed according to the local law.

13 Symbol Instructions

 Manufacturer's logo	 Type B applied part	 Refer to instruction manual/ booklet
 Environment-friendly use period	 Manufacturer	 Use-by date
 Serial number	 Do not dispose of the product into the ordinary municipal waste or garbage system	 Caries Detection Mode
 Caution	 Atmospheric pressure limitation	 CE marking
 Fragile, handle with care	 Rotating plug	 UDI Unique device identifier
 Humidity limitation	 Temperature limit	
 This way up	 Medical Device	
 Keep dry	 Class II equipment	
 Direct current	 Alternating current	
 Full Power Mode	 Progressive Mode	
 Pulsed Mode	 Battery Indicator	
 Ultra High Power Mode	 High Power Mode	
 Standard Power Mode	 On/Off Button	
 Mode/Time Button	 Date of manufacture	

14 Statement

All rights of modifying industrial design, inner structure, instruction manual, etc, of the product are reserved to the manufacturer without further notice. The pictures are only for reference. The final interpretation rights belong to Guilin Veirun Medical Technology Co.,Ltd..

15 Attachment Lists

No.	Attachment Name	Pcs
1	main unit	1
2	shading plate(options available)	1
3	power adapter with one USB cable	1
4	charger cradle	1
5	rechargeable lithium battery	1
6	light source	1
7	disposable sleeves	50
8	light-curing height block	1

NOTE: The exactly specifications of accessories are not been shown detailedly in this operation instrument. See the attached page and packing list for more information.

16 EMC

Note:

- (1) Unauthorized changes or modifications without the affirmative consent of Guilin Veirun Medical Technology Co.,Ltd. may cause EMC problems to the product or other equipment.**
- (2) The DV-50 LED light curing device has been tested and homologated in accordance with operating procedures related to EMC.**

16.1 Requirements of cable installation

Cable Name	Cable Type	Cable Length
Powre supply output line.	Unshielded parallel line.	1 meter.

16.2 Key parts of EMC

Key parts of EMC of the product are LED driver chip and the power adapter. Using or replacing accessories which are not designed and supplied by our company would result in performance degradation of electromagnetic emissions and electromagnetic immunity. Therefore, do not replace parts of the product without permission.

16.3 Guidance and Manufacturer's Declaration--Electromagnetic Emissions

Guidance and Manufacturer's Declaration--Electromagnetic Emissions.		
The DV-50 LED light curing device is indicated for use in the electromagnetic environment specified below. The customer or the use of the models DV-50 LED light curing device should assure that it is used in such an environment.		
Emissions test	Compliance	Electromagnetic environment --guidance.
RF emissions GB 4824-2019	Group 1	The models DV-50 LED light curing device use RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions GB 4824-2019	Group B	The models DV-50 LED light curing device are suitable for used in domestic establishment and in establishment directly connected to a low voltage power supply network which supplies buildings used for domestic purposes.

Harmonic emissions GB 17625.1-2012	Not applicable	
Voltage fluctuations /flicker emissions GB 17625.2-2007	Applicable	


16.4 Guide and Manufacturer's Statement--Electromagnetic Immunity.

Guide and Manufacturer's Statement--Electromagnetic Immunity			
The DV-50 LED light curing device is indicated for use in the electro-magnetic environment specified below. The customer or the use of the models DV-50 LED light curing device should assure that it is used in such an environment.			
Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment--Guidance.
Electrostatic discharge(ESD) GB/T 17626.2-2018	± 6 kV contact ± 6 kV contact	± 6 kV contact ± 6 kV contact	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst GB/T 17626.4-2018	± 2 kV for power supply lines ± 1 kV for input/output lines	± 2 kV for power supply lines ± 1 kV for interconnecting cable	Mains power quality should be that of a typical commercial or hospital environment.

Surge GB/T 17626.5–2019	± 1 kV line to line ± 2 kV line to earth	± 1kV line to line	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines GB/T 17626.11–2016	<5%U _T (> 95% dip in U _T) for 0.5 cycle 40% U _T (60% dip in U _T) for 5 cycles 70% U _T (30% dip in U _T) for 25 cycles <5%U _T (95% dip in U _T) for 5 sec.	<5%U _T (> 95% dip in U _T) for 0.5 cycle 40% U _T (60% dip in U _T) for 5 cycles 70% U _T (30% dip in U _T) for 25 cycles <5%U _T (95% dip in U _T) for 5 sec.	Mains power quality should be that of a typical commercial or hospital environment. If the user of the models DV–50 LED light curing device require continued operation during power mains interrup tions,it is recom mended that the models DV–50 LED light curing device be powered from an nonnot rruptible powersupply or a battery.
Power frequency (50/60 Hz) magnetic field GB/T 17626.8–2006	3 A/m	3 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
Note:U _T is the a.c. Mains voltage prior to application of the test level.			

16.5 Guide and Manufacturer's Statement--Electromagnetic Immunity.

Guide and Manufacturer's Statement--Electromagnetic Immunity			
The DV–50 LED light curing device is indicated for use in the electro–magnetic environment specified below. The customer or the use of the models DV–50 LED light curing device should assure that it is used in such an environment.			
Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment--Guidance
Conducted RF GB/T 17626.6–2017	3 Vrms 150 kHz~ 80 MHz	3 Vrms	Portable and mobile RF communications equipment should be used no closer to any part of the models DV–50 LED light curing device, including cables,than the recom mended separation distance calculated from the frequency of the transmitter. Recommended Separation Distance. $d = \left[\frac{3.5}{V_1} \right] \sqrt{p}$ $d = \left[\frac{3.5}{E_1} \right] \sqrt{p} \quad 80\text{MHz} \sim 800\text{MHz}$ $d = \left[\frac{7}{E_1} \right] \sqrt{p} \quad 800\text{MHz} \sim 2.5\text{GHz}$ Where P is the maximum output power rating of the transmitter In watts(W) according to the transmitter manufacturer and d is the recommended separation distance in meters(m)
Radiated RF GB/T 17626.3–2016	3 V/m 80 MHz~ 2.5 GHz	3 V/m	

			<p>Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey, should be less than the compliance level in each frequency range.^b</p> <p>Interference may occur in the vicinity of equipment marked with the following symbol:</p> 
--	--	--	--

Note1: At 80 MHz and 800 MHz, the higher frequency range applies.

Note2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

^aField strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the models DV-50 LED light curing device are used exceeds the applicable RF compliance level, the model DV-50 LED light curing device level should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the models DV-50 LED light curing device.

^bOver the frequency range 150 KHz to 80 MHz, field strengths should be less than 3 V/m.

16.6 Recommended separation distances between portable and mobile RF communications equipment and the models DV-50 LED light curing device.

Recommended separation distances between portable and mobile RF communications equipment and the models DV-50 LED light curing device.

<p>The models DV-50 LED are intended for use in electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the models DV-50 LED can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the models DV-50 LED are recommended below, according to the maximum output power of the communications equipment.</p>			
Rated maximum output power of transmitter/W.	Separation distance according to frequency of transmitter/m.		
	150 kHz~ 80 MHz	80 MHz~800 MHz	800 MHz~2.5 GHz
	$d = \left[\frac{3.5}{V_1}\right]\sqrt{p}$	$d = \left[\frac{3.5}{E_1}\right]\sqrt{p}$	$d = \left[\frac{7}{E_1}\right]\sqrt{p}$
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23

For transmitter rated at a maximum output power not listed above, the recommended separation distance d in meters(m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts(W) accordable to the transmitter manufacturer.

Note1: At 80 MHz and 800 MHz, the higher frequency range applies.

Note2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

The DV-50 LED light curing device has passed tests according IEC 60601-1-2, but it is no guarantee of immunity from electromagnetic interference. Avoid using DV-50 LED light curing device in high electromagnetic environment.